


TEST REPORT

(Electronic version)

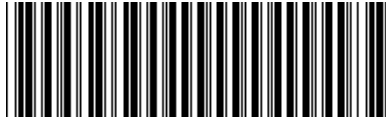

No: 200255156

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: RIGR-6838-04

ISSUE DATE: 2020-08-18

扫码下载报告



APPLICANT: DIGITAL MEDIA SAC
ADDRESS: LAS ANTARAS M25 CHORRILLOS - LIMA- PERU

INFORMATION CONFIRMED BY APPLICANT:

FLAT KN95 MASK
QUANTITY: 40 PIECES
BRAND: ADN PERU
MODEL: SK0720
MANUFACTURE'S NAME: ADN PERU EIRL

DATE RECEIVED/DATE TEST STARTED: 2020-08-11

CONCLUSION:

HEAD BAND	M
VISUAL FIELD	M
FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M
FLAMMABILITY	M
DEAD SPACE	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
"----" -NO COMMENT

REMARK:

ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:
Yuan Liu ENGINEER

刘圆




PAGE 1 OF 4

TEST REPORT

(Electronic version)

No:200255156

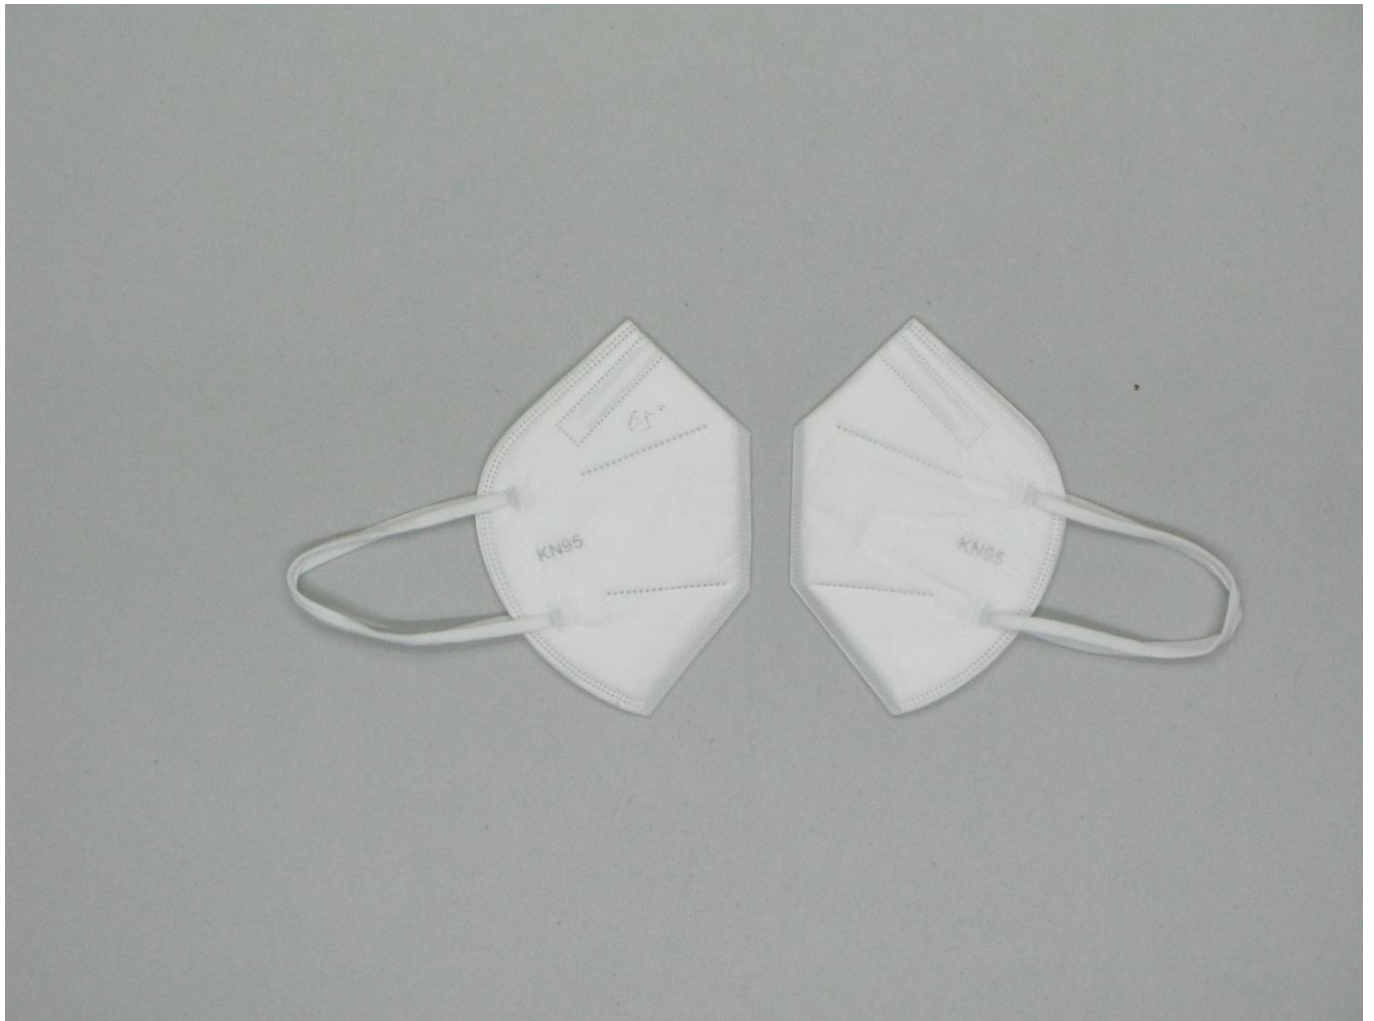

TEST REPORT

(Electronic version)

No:200255156

HEAD BAND

(GB 2626-2006 6.11)

UNTREATED SAMPLE:
1# PASS
CONDITIONING TREATED:
1# PASS

REQUIREMENT
EACH HEAD BAND, BUCKLE AND OTHER ADJUST
PARTS OF MASK SHOULD NOT SLIP OR BREAK
UNDER 10N TENSION FOR 10S.
(GB 2626-2006)

VISUAL FIELD(°)

(GB 2890-2009 6.8)

70

REQUIREMENT
≥60
(GB 2626-2006)

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER(%)

(GB 2626-2006 6.3, AIR FLOW:85L/min, AEROSOL:NaCl, AEROSOL CONCENTRATION:15mg/m³,
TEMP:24.3℃ RH:34.6%)

FILTRATION EFFICIENCY:
UNTREATED SAMPLE
1# 99.749
2# 99.708
3# 99.719
4# 99.723
5# 99.711
6# 99.734
7# 99.692
8# 99.741
9# 99.688
10# 99.728
CONDITIONING TREATED
1# 99.676
2# 99.641
3# 99.608
4# 99.632
5# 99.611

REQUIREMENT
FILTRATION EFFICIENCY:
≥95.0
(KN95)
(GB 2626-2006)

INSPIRATORY RESISTANCE(Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:
1# 156.8
2# 154.3
PRETREATMENT SAMPLE:
1# 148.3
2# 147.6

REQUIREMENT
≤350
(GB 2626-2006)

EXPIRATORY RESISTANCE(Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:
1# 143.9
2# 141.2
PRETREATMENT SAMPLE:
1# 136.8
2# 134.5

REQUIREMENT
≤250
(GB 2626-2006)



PAGE 3 OF 4

TEST REPORT

(Electronic version)

No:200255156

FLAMMABILITY(s)

(GB 2626-2006 6.15)

AFTERFLAME TIME
UNTREATED SAMPLE
1# 0.0
2# 0.0
CONDITIONING TREATED
3# 0.0
4# 0.0

REQUIREMENT
AFTERFLAME TIME
≤5
(GB 2626-2006)

DEAD SPACE

(GB 2626-2006 6.9)

CARBON DIOXIDE VOLUME FRACTION:
0.7%

REQUIREMENT
CARBON DIOXIDE VOLUME FRACTION SHOULD
NOT BE MORE THAN 1%
(GB 2626-2006)



—End of Report—

PAGE 4 OF 4